

# Test Report

**Applicant:** Wenzhou Jiada Technology Co., Ltd  
**Address:** No.401, Building 19th, Rainbow Wisdom Park, Longgang City, Cangnan Area, Wenzhou City, Zhejiang Province, China.

**The following sample(s) was/were submitted and identified on behalf of the client as:**

Product name: FILTERING HALF MASK  
Model: JD-99(G)  
Trade mark: JIADA  
Manufacturer: Wenzhou Jiada Technology Co., Ltd  
Address: No.401, Building 19th, Rainbow Wisdom Park, Longgang City, Cangnan Area, Wenzhou City, Zhejiang Province, China.  
Classification: FFP2 NR  
Sample quantity: 69 Pcs

Sample Received Date: Mar. 17, 2021  
Testing Period: Mar. 17, 2021~ Mar. 24, 2021

**Test Requirement:**

According to the requirement of the client, the test item(s) of the sample is according to the standard EN 149:2001+A1:2009.

**Test Result(s):** Please refer to the following page(s)

**Test Method:** Please refer to the following page(s)

Compiled by: \_\_\_\_\_

Reviewed by: \_\_\_\_\_

Approved by: \_\_\_\_\_

Date: \_\_\_\_\_

2021-03-24

**Summary of assessment\***

Clause	Assessment
7.9.2 Penetration of filter material	Pass
7.11 Flammability	Pass
7.12 Carbon dioxide content of the inhalation air	Pass
7.16 Breathing resistance	Pass

**Key**

Pass	Requirement satisfied.
NRq	The clauses were not required.
Fail	Requirement not satisfied. Refer to the "Result details" section for more information.
N.A.	Requirement not applicable.

Test	Uncertainty
Penetration of filter material (NaCl)	1.60 %
Penetration of filter material (Paraffin Oil)	1.78 %
Carbon dioxide content of the inhalation air	5.34 %
Breathing resistance (30 L/min)	3.60 %
Breathing resistance (95 L/min)	2.20 %
Breathing resistance (160 L/min)	2.00 %

\* Assessment relates only to those specimens which were tested and subjects in this report.

## Test Result

### Clause 7.9.2 Penetration of Filter Material

(EN 149:2001+A1:2009, Clause 8.11)

Test Requirement			Results	Comment
The penetration of the filter of the particle filtering half mask shall meet the requirements of the following table.			Detail refer to Appendix 1	Pass
Classification	Maximum penetration of test aerosol(%)			
	Sodium chloride test 95 L/min	Paraffin oil test 95 L/min		
FFP1	20	20		
FFP2	6	6		
FFP3	1	1		

**Appendix 1: Summarization of Test Data**

Penetration of filter material

Aerosol	Condition	Sample No.	Penetration (%)		Assessment
			Average in 30s after 3 min	Max. during exposure	
Sodium chloride test	A.R.	1#	0.87	/	Pass
		2#	0.81	/	
		3#	0.83	/	
	S.W.	7#	0.84	/	
		8#	0.82	/	
		9#	0.82	/	
	M.S. + T.C.	13#	/	1.19	
		14#	/	1.15	
		15#	/	1.13	
Paraffin oil test	A.R.	4#	1.98	/	
		5#	1.96	/	
		6#	1.91	/	
	S.W.	10#	2.22	/	
		11#	1.98	/	
		12#	1.35	/	
	M.S. + T.C.	16#	/	2.21	
		17#	/	2.68	
		18#	/	2.09	
Flow rate of test aerosol: 95.0 L/min					

**Clause 7.11 Flammability**

(EN 149:2001+A1:2009, Clause 8.6)

Test Requirement	Results	Comment
The material used shall not present a danger for the wearer and shall not be of highly flammable nature when tested, the particle filtering half mask shall not burn or not to continue on burn for more than 5 s after removal from the flame.	Detail refer to Appendix 2	Pass

**Appendix 2: Summarization of Test Data**

Flammability

Condition	Sample No.	Result	Assessment
A.R.	31#	Flammable, burn for no more than 5 s	Pass
	32#	Flammable, burn for no more than 5 s	
T.C.	33#	Flammable, burn for no more than 5 s	
	34#	Flammable, burn for no more than 5 s	

**Clause 7.12 Carbon Dioxide Content of The Inhalation Air**

(EN 149:2001+A1:2009, Clause 8.7)

Test Requirement	Results	Comment
The carbon dioxide content of the inhalation air (dead space) shall not exceed an average of 1.0 % (by volume).	Detail refer to Appendix 3	Pass

**Appendix 3: Summarization of Test Data**

Carbon Dioxide Content of The Inhalation Air

Condition	Sample No.	Result	Assessment
A.R.	19#	0.43%	Pass
	20#	0.39%	
	21#	0.39%	
		Mean value: 0.40%	

**Clause 7.16 Breathing Resistance**

EN 149:2001+A1:2009, Clause 8.9)

Test Requirement				Results	Comment
The breathing resistances apply to valved and valveless filtering half masks and shall meet the requirements as the following table.				Detail refer to Appendix 4	Pass
Classification	Maximum permitted resistance (mbar)				
	Inhalation		Exhalation		
	30 L/min	95 L/min	160 L/min		
FFP1	0.6	2.1	3.0		
FFP2	0.7	2.4	3.0		
FFP3	1.0	3.0	3.0		

**Appendix 4: Summarization of Test Data**

Specimen	Condition	Inhalation(mbar)		Exhalation resistance(mbar)				
		At 30 L/min	At 95 L/min	At 160 L/min				
				A	B	C	D	E
22#	A.R.	0.38	1.33	2.01	2.01	2.00	1.99	1.99
23#		0.37	1.33	2.01	2.00	2.01	2.00	1.99
24#		0.39	1.34	2.02	2.02	2.01	2.01	2.00
25#	S.W.	0.39	1.34	2.02	2.01	2.02	2.01	2.00
26#		0.39	1.33	2.02	2.01	2.01	2.00	2.00
27#		0.40	1.34	2.03	2.02	2.03	2.02	2.01
28#	T.C.	0.36	1.29	1.92	1.91	1.92	1.91	1.90
29#		0.35	1.28	1.91	1.90	1.91	1.90	1.89
30#		0.36	1.30	1.92	1.91	1.92	1.91	1.90
/	F.C.	/	/	/	/	/	/	/
/		/	/	/	/	/	/	/
/		/	/	/	/	/	/	/

A: facing directly ahead; B: facing vertically upwards; C: facing vertically downwards; D: lying on the left side; E: lying on the right side

**Sample photo(s):**

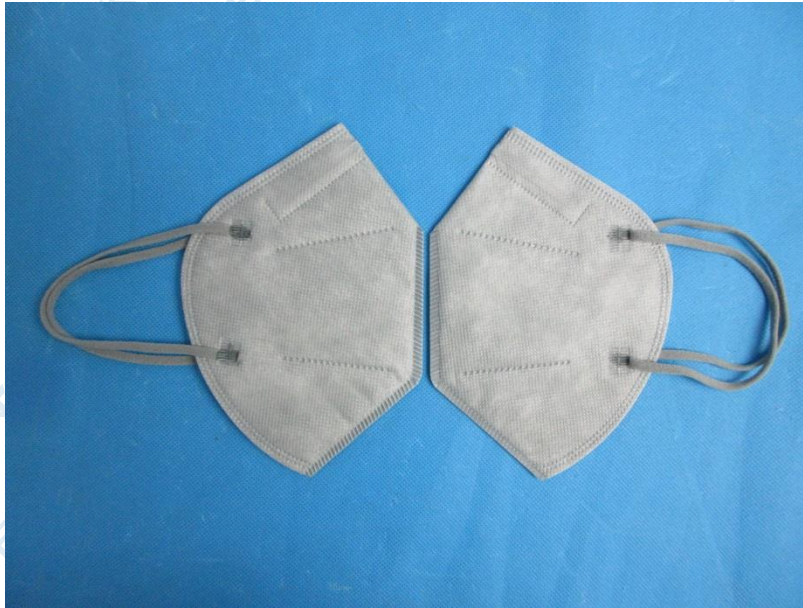


Fig.1



Fig.2

\*\*\*\*End of Report\*\*\*\*

The test report is effective only with both signature and specialized stamp, the result(s) shown in this report refer only to the sample(s) tested. Without written approval of NTEK, this report can't be reproduced except in full; The laboratory is not responsible for the authenticity of the sample information provided by the customer; The laboratory is not responsible for any deviation of results due to methods/standards provided by the customer.